



Research  
Medical Instrumentation—Article

## Quality Monitoring of Porous Zein Scaffolds: A Novel Biomaterial

Yue Zhang, Wei-Ying Li, Run Lan, Jin-Ye Wang \*

School of Biomedical Engineering, Shanghai Jiao Tong University, Shanghai 200240, China

### ARTICLE INFO

#### Article history:

Received 30 June 2016

Revised 15 November 2016

Accepted 13 December 2016

Available online 20 January 2017

#### Keywords:

Zein

Amino acid analysis

SDS-PAGE

Gamma-ray sterilization

MTT assay

CCK-8 assay

### ABSTRACT

Our previous studies have shown that zein has good biocompatibility and good mechanical properties. The first product from a porous scaffold of zein, a resorbable bone substitute, has passed the biological evaluation of medical devices (ISO 10993) by the China Food and Drug Administration. However, Class III medical devices need quality monitoring before being placed on the market, and such monitoring includes quality control of raw materials, choice of sterilization method, and evaluation of biocompatibility. In this paper, we investigated four sources of zein through amino acid analysis (AAA) and sodium dodecyl sulfate polyacrylamide gel electrophoresis (SDS-PAGE) in order to monitor the composition and purity, and control the quality of raw materials. We studied the effect of three kinds of sterilization method on a porous zein scaffold by SDS-PAGE. We also compared the changes in SDS-PAGE patterns when irradiated with different doses of gamma radiation. We found that polymerization or breakage did not occur on peptide chains of zein during gamma-ray ( $\gamma$ -ray) sterilization in the range of 20–30 kGy, which suggested that  $\gamma$ -ray sterilization is suitable for porous zein scaffolds. Regarding cell compatibility, we found a difference between using a 3-(4,5-dimethylthiazol-2-yl)-2,5-diphenyl tetrazolium bromide (MTT) assay and a cell-counting kit-8 (CCK-8) assay to assess cell proliferation on zein film, and concluded that the CCK-8 assay is more suitable, due to its low background optical density.

© 2017 THE AUTHORS. Published by Elsevier LTD on behalf of the Chinese Academy of Engineering and Higher Education Press Limited Company. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

### 1. Introduction

Zein is one of the major storage proteins of corn, and is the main byproduct in the corn-processing industry [1]. Its unique hydrophobicity causes researchers to study it for possible applications beyond the food industry [2]. Our group is the first to study zein as a biomaterial in tissue engineering, and we have proved its good biocompatibility and mechanical properties. The first product from a porous scaffold of zein may be used as a bone substitute [3–6]. As a Class III medical device, quality monitoring for raw materials, a suitable sterilization method, and biocompatibility are required.

Firstly, the quality of the raw materials must be stable and controllable. We found that zein purchased from different sources had a different appearance, affecting its scaffold shaping and mechanical properties; this prompted us to investigate the differences in zein from different sources.

Sterilization process control is important for the quality management system of sterile medical device manufacturers. The control level of the sterilization directly affects the quality and safety of the sterile medical devices. The most traditional method of sterilization for manufacturers is ethylene oxide sterilization. However, this method may cause the problem of ethylene oxide residue in the porous scaffolds [7,8]. Therefore, we investigated other traditional methods such as moist-heat sterilization, dry-heat sterilization, and gamma-ray ( $\gamma$ -ray) sterilization. However, these methods may also be problematic for the structural stability of zein because heat and pressure may influence the structure of zein [9]. For example, the use of gamma radiation involves a great deal of energy, which may cause molecule ionization [10].

A traditional way to assess the proliferation of cells is a 3-(4,5-dimethylthiazol-2-yl)-2,5-diphenyl tetrazolium bromide (MTT) assay [11,12], a method that we have applied in our previous work [3–6].

\* Corresponding author.

E-mail address: [jinyewang@sjtu.edu.cn](mailto:jinyewang@sjtu.edu.cn)

Recently, we found that the background optical density (OD) of zein scaffolds was significantly high in MTT assays, which may affect the evaluation of data [13,14]. Therefore, we tried another method, a cell-counting kit-8 (CCK-8) assay [15], and compared these two methods in the evaluation of cell proliferation on zein film. We also considered possible factors causing a high background OD of zein in the MTT assay.

## 2. Materials and methods

### 2.1. Amino acid analysis, sodium dodecyl sulfate polyacrylamide gel electrophoresis, and microscopy characterization

Zein 1 was purchased from Kobayashi Perfumery Co., Ltd. (Japan), zein 2 (260-01283) and zein 3 (261-00015) were both purchased from Wako Pure Chemical Industries, Ltd. (Japan), and zein 4 (in sheet form) was purchased from Wujiang Bache Pharmaceutical Adjuvant Co. (China). We obtained the zein 4 powders by grinding sheets of zein 4 using a grinder (Q-100A2, Shanghai Bingdu Electric Co., Ltd., China) and then sifting. All were dispersed in 6 mol·L<sup>-1</sup> HCl with a ratio of 1:6 (g·mL<sup>-1</sup>). The mixture was kept in an oil bath at 110 °C for 22 h. After acidolysis, the mixture was first rotary evaporated to concentrate it, and then lyophilized (FreeZone 4.5, Labconco, USA) to obtain the powder. The powder was dissolved in citric acid-sodium citrate buffer (pH = 2.2) and analyzed using a High-Speed Amino Acid Analyzer (L-8900, Hitachi, Japan) [16].

Samples of the four sources of zein were dissolved in 75 wt% ethanol solution at a concentration of 1 mg·mL<sup>-1</sup>. Next, 20 µL of the sample solution was mixed with 20 µL of the loading buffer, and the mixture was heated in a water bath at 90 °C for 15 min. The loading buffer was made of 2 mL glycerol, 2 mL 10 wt% sodium dodecyl sulfate (SDS), 1 mL 2-mercaptoethanol, 0.5 mL 0.1% bromophenol blue, and 0.625 mL stacking gel buffer. Denaturing gel electrophoresis was carried out with a vertical slab gel apparatus (Bio-Rad, USA). The gel was made of a stacking gel of 5% and a resolving gel of 12% acrylamide concentration. It was run at room temperature at 110 V for 30 min and then at 150 V for about 1 h, using a running buffer made of 3.05 g of Tris base, 14.4 g of glycine, and 1 g of SDS dissolved in 1 L of Milli-Q water. The bands were visualized by Coomassie blue R250 staining [17].

The micro-morphology of the zein powders was investigated using scanning electron microscopy (SEM) (S-3400N, Hitachi, Japan) and fluorescence microscopy (IX71, Olympus, Japan) with an optical filter (U-MSWB2, Olympus, Japan) to produce the excitation light.

### 2.2. Porous zein scaffolds: Fabrication and sterilization

Zein 1 was mixed with sodium chloride (particle sizes from 0.3 mm to 0.425 mm) at a mass ratio of 1:1.5, and the mixture was molded into 3D scaffolds using a stainless steel mold ( $\phi = 1.75$  mm) at 0.1 MPa for 2 min on both sides. Next, the scaffolds were leached in a water bath at 55 °C for 30 min, cut to a cylindrical rod with a diameter of 2 mm and a height of 4 mm, and lyophilized for 6 h [4].

$\gamma$ -ray sterilization was performed by keeping porous zein scaffolds under 20 kGy, 25 kGy, and 30 kGy [18]. The zein powder and the porous zein scaffolds were monitored by sodium dodecyl sulfate polyacrylamide gel electrophoresis (SDS-PAGE) before and after sterilization.

Dry-heat sterilization was performed by keeping the zein powder in an electro-thermostatic blast oven (DHG-9053A, Shanghai Jing Hong Laboratory Instrument Co., Ltd., China) at 160 °C for 3 h. Moist-heat sterilization was performed by keeping the zein powder in an autoclave sterilizer (HVE-50, Hirayama, Japan) at 121 °C for 20 min. The zein powders were monitored by SDS-PAGE before and after sterilization.

### 2.3. Cell culture and proliferation

L929 cells (Type Culture Collection of the Chinese Academy of Sciences, China) were used in cell studies and cultured in GIBCO® Dulbecco's Modified Eagle Medium (DMEM) (Life Technologies Co., USA) supplemented with 10% newborn calf serum (Shanghai Yuanmu Biological Technology Co., Ltd., China) and antibiotics (100 U·mL<sup>-1</sup> penicillin and 100 µg·mL<sup>-1</sup> streptomycin) (Sinopharm Chemical Reagent Co., Ltd., China) in a 37 °C 5% CO<sub>2</sub> incubator (NU-4750E, NuAire, Ltd., USA).

Zein film slides were made by coating 10 µL of zein 1 glacial acetic acid solution at a concentration of 0.1 g·mL<sup>-1</sup> on a glass slide of 8 mm in diameter. Before cell seeding, all slides were sterilized at 160 °C for 3 h, and then immersed in culture medium for 2 h in 48-well plates. L929 cells were seeded at a density of  $2 \times 10^4$  mL<sup>-1</sup> on both glass slides and zein film slides, and 500 µL of the cell suspension was added to each test well, while 500 µL of the culture medium was added to each background well. The plates were incubated for 6 d.

### 2.4. MTT and CCK-8 assays

The proliferation of L929 cells on glass slides and zein film slides was assessed using an MTT assay and a CCK-8 assay. Before assessment, the solution in each test or background well was replaced with 500 µL of culture medium. Then 50 µL of MTT (AMRESCO, USA) at a concentration of 5 mg·mL<sup>-1</sup>, or a CCK-8 kit (YEASEN, China), was added to each well, and the plates were incubated for another 4 h. After incubation, 100 µL of the solution per well was transferred to a 96-well plate for the CCK-8 assay, while for the MTT assay, the solution was replaced with 300 µL of dimethyl sulfoxide (DMSO) and transferred to a 96-well plate at 150 µL per well, after shaking for 10 min. The OD of the plate was measured at 450 nm ( $n = 6$ ) using a microplate photometer (Multiskan FC, Thermo Scientific, USA) for the CCK-8 assay, and at 490 nm ( $n = 6$ ) for the MTT assay. After measurement, the wells for the CCK-8 assay were washed carefully with phosphate-buffered saline (PBS) solution; 500 µL of culture medium was then added per well to continue incubating. The assays were assessed at the same time every day for 6 d.

To investigate the background in the MTT assay, zein film slides and glass slides were immersed in culture medium or PBS for 12 h. After being incubated with or without MTT for another 4 h, the solution was replaced with 300 µL of DMSO and transferred to a 96-well plate at 150 µL per well, after shaking for 10 min. Next, the OD of the plate was measured at 490 nm ( $n = 6$ ).

### 2.5. Statistical analysis

Where applicable, all data were expressed as means  $\pm$  standard deviation ( $n = 6$ ). The significance of the differences between data was assessed by one-way analysis of variance (ANOVA). Statistical significance was set at  $P < 0.05$ .

## 3. Results and discussion

### 3.1. Characterization of four sources of zein

In appearance, both zein 1 and zein 2 are white, while zein 3 and zein 4 are yellow. The morphologies of the zein powders from the four sources could easily be observed due to the autofluorescence of zein protein, as shown in Fig. 1(a–d). As this figure shows, the powders of both zein 1 and zein 2 are pebble-like, while the powders of zein 3 and zein 4 are clastic. Regarding the size of the powders, the subsize powder of zein 3 appears to be

much more prevalent than in zein 1 or zein 2, and much smaller in size. The SEM images shown in Fig. 1(e–h) show that both zein 1 and zein 2 have smooth surfaces, while both zein 3 and zein 4 are porous.

We then investigated the amino acid composition of the four sources of zein, as shown in Table 1. Fig. 2 shows the liquid chromatogram of zein 1 as a typical chromatogram of zein. Table 1 shows that even though the zein from the four sources differs somewhat in morphology, there is no significant difference in amino acid composition. Since the major amino acid composition of zein is glutamic acid ( $24.8\% \pm 0.3\%$ ), leucine ( $19.2\% \pm 0.4\%$ ), proline ( $9.8\% \pm 0.3\%$ ), and alanine ( $9.6\% \pm 0.1\%$ ), which are all hydrophobic amino acids, it is reasonable for zein to be a hydrophobic protein.

Fig. 3 shows the electrophoretograms of the four sources of zein. These show two major bands at 25 kDa and 22 kDa in all four sources of zein, with no significant differences.

### 3.2. SDS-PAGE before and after sterilization

Fig. 4 shows the electrophoretograms of the zein before and after thermal sterilization, and Table 2 provides the intensity analysis for Fig. 4. No new bands appeared after sterilization, which indicates that polymerization or breakage did not occur on peptide chains of the zein when suffering dry-heat sterilization and moist-heat sterilization. The results suggest that both sterilization methods are acceptable. Table 2 shows that the proportion of band 1, the larger molecular weight (25 kDa), is lower than the proportion of band 2, the smaller molecular weight (22 kDa).

Fig. 5 shows the electrophoretograms of the zein before and after  $\gamma$ -ray sterilization, and Table 3 provides the intensity analysis for Fig. 5. No new bands were produced, although the relative percentage of the two bands was slightly different in the 30 kGy dosage. Thus, gamma radiation of 25 kGy, which is the recommended dosage, is suitable for the sterilization of zein scaffolds [18].

### 3.3. Cell proliferation

Fig. 6 shows the L929 cell proliferation on glass and zein film. We found that the curves obtained from the MTT assay and CCK-8

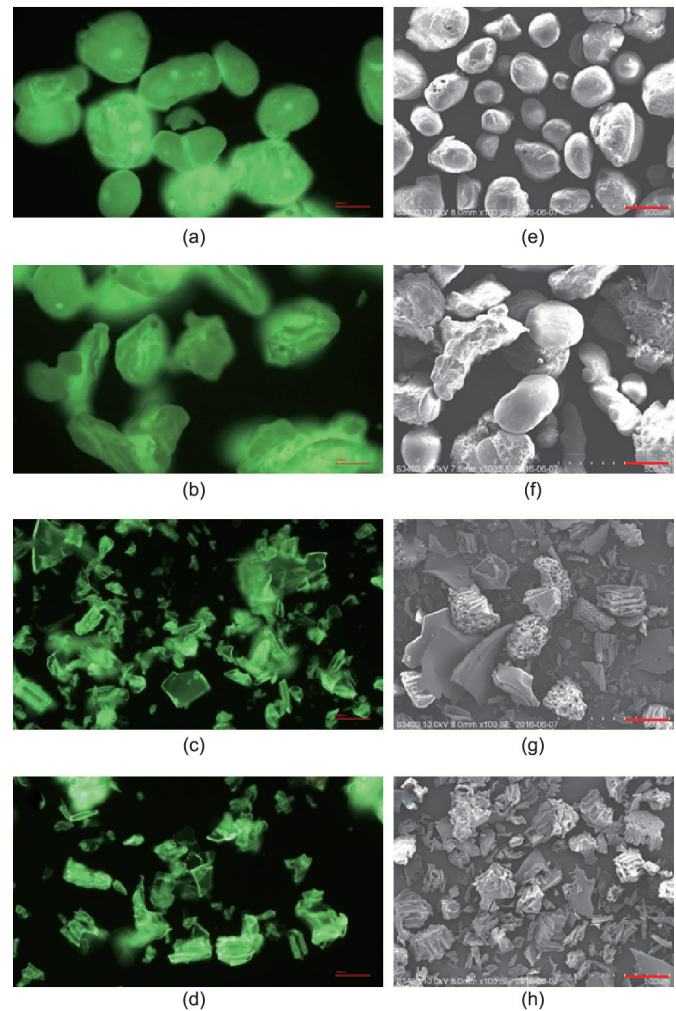


Fig. 1. Images of zein powders. Fluorescence microscope images of (a) zein 1, (b) zein 2, (c) zein 3, and (d) zein 4; SEM images of (e) zein 1, (f) zein 2, (g) zein 3, and (h) zein 4. The scale bar on each image represents 200  $\mu\text{m}$ .

Table 1  
Amino acid composition of four zein sources.

Amino acid	Zein 1		Zein 2		Zein 3		Zein 4	
	ng·mg <sup>-1</sup>	%	ng·mg <sup>-1</sup>	%	ng·mg <sup>-1</sup>	%	ng·mg <sup>-1</sup>	%
Asp	31 076.188	5.2	31 797.767	5.3	29 592.712	5.3	30 082.844	5.3
Thr	15 271.866	2.5	15 167.695	2.6	15 094.554	2.7	13 962.363	2.5
Ser	31 716.602	5.3	31 694.453	5.3	29 706.826	5.3	27 307.124	4.8
<b>Glu</b>	<b>150 275.829</b>	<b>25.1</b>	<b>147 218.050</b>	<b>24.8</b>	<b>140 754.298</b>	<b>25.0</b>	<b>137 978.168</b>	<b>24.5</b>
Gly	6 514.847	1.1	6 666.862	1.1	5 702.660	1.0	5 629.660	1.0
<b>Ala</b>	<b>57 419.553</b>	<b>9.6</b>	<b>57 646.861</b>	<b>9.7</b>	<b>53 655.466</b>	<b>9.5</b>	<b>54 780.573</b>	<b>9.7</b>
Val	17 211.984	2.9	15 008.123	2.5	17 173.698	3.1	15 789.398	2.8
Cys	7 857.047	1.3	11 607.190	2.0	6 596.639	1.2	12 912.832	2.3
Met	6 565.298	1.1	9 777.207	1.6	9 057.595	1.6	9 544.431	1.7
Ile	17 782.280	3.0	14 804.524	2.5	17 557.566	3.1	15 741.966	2.8
<b>Leu</b>	<b>118 507.485</b>	<b>19.8</b>	<b>111 625.500</b>	<b>18.8</b>	<b>107 670.201</b>	<b>19.2</b>	<b>108 041.489</b>	<b>19.2</b>
Tyr	29 833.976	5.0	29 885.841	5.0	26 706.572	4.8	26 592.639	4.7
Phe	39 886.276	6.7	39 603.144	6.7	36 414.309	6.5	37 373.132	6.6
Lys	428.899	0.1	129.941	0.0	0.000	0.0	0.000	0.0
His	5 043.198	0.8	5 330.143	0.9	4 837.169	0.9	4 404.220	0.8
Arg	7 262.791	1.2	7 431.617	1.2	7 502.331	1.3	7 323.227	1.3
<b>Pro</b>	<b>56 749.686</b>	<b>9.5</b>	<b>59 291.397</b>	<b>10.0</b>	<b>54 119.886</b>	<b>9.6</b>	<b>56 719.073</b>	<b>10.1</b>

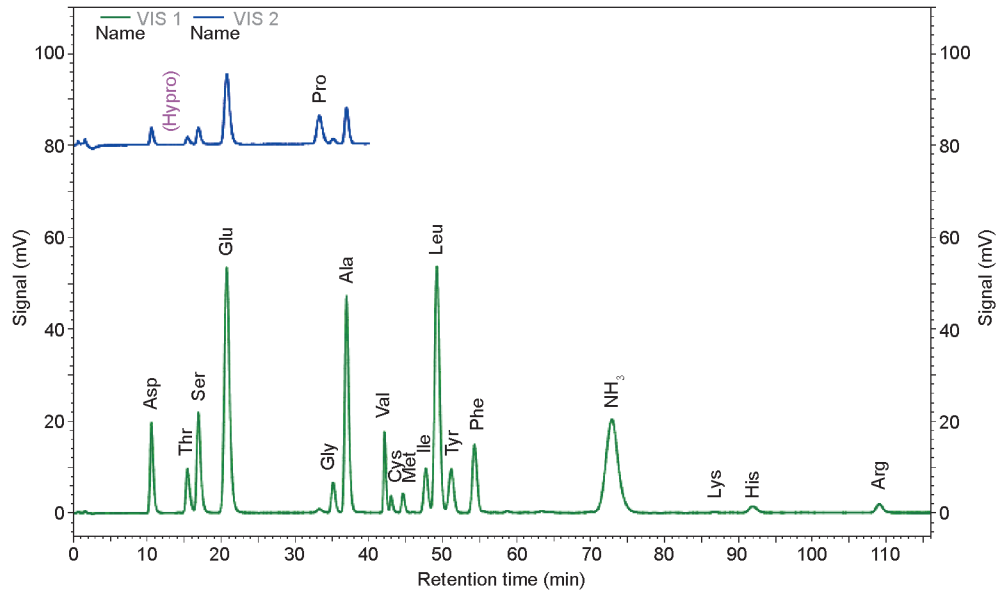


Fig. 2. Chromatogram of zein 1.

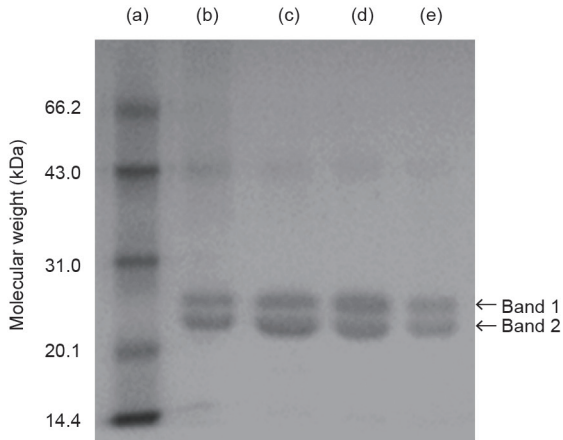


Fig. 3. SDS-PAGE images of zein from different suppliers. (a) The marker; (b) zein 1; (c) zein 2; (d) zein 3; (e) zein 4.

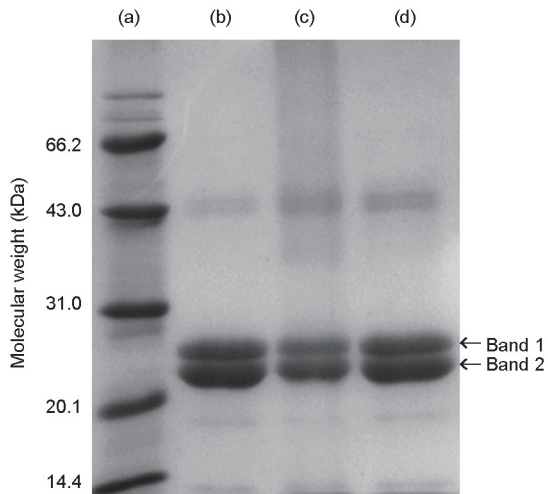


Fig. 4. SDS-PAGE images using different sterilization methods. (a) The marker; (b) zein 2 before sterilization; (c) zein 2 treated by dry-heat sterilization; (d) zein 2 treated by moist-heat sterilization.

Table 2  
Intensity analysis for Fig. 4.

Bands	Band 1 (25 kDa)		Band 2 (22 kDa)	
	µg	%	µg	%
(b)	1.90	45.9	2.24	54.1
(c)	1.33	45.7	1.72	54.3
(d)	1.85	45.7	2.20	54.3

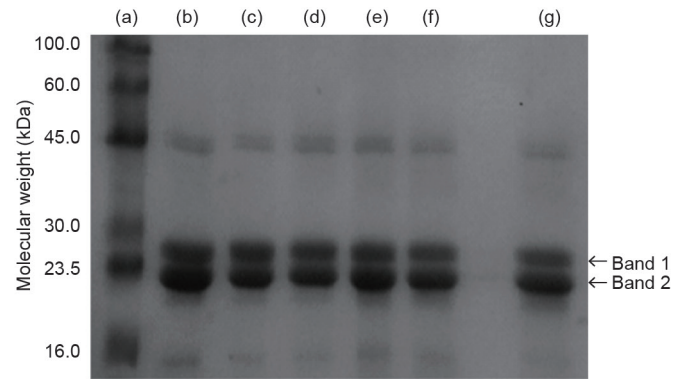


Fig. 5. SDS-PAGE images before and after  $\gamma$ -ray sterilization. (a) The marker; (b) zein 2; (c) zein 3; (d) zein 4; (e) the porous zein (zein 2) scaffolds sterilized with 20 kGy; (f) the porous zein (zein 2) scaffolds sterilized with 25 kGy; (g) the porous zein (zein 2) scaffolds sterilized with 30 kGy.

Table 3  
Intensity analysis for Fig. 5.

Bands	Band 1 (25 kDa)		Band 2 (22 kDa)	
	µg	%	µg	%
(b)	1.69	43.3	2.21	56.6
(c)	1.49	43.3	1.95	56.6
(d)	1.39	43.3	1.82	56.6
(e)	1.43	41.4	2.02	58.6
(f)	1.28	41.6	1.80	58.4
(g)	1.02	35.5	1.85	64.5

assay were slightly different. The MTT assay showed that L929 cells proliferated better on zein film than on glass from the second day after seeding, while the CCK-8 assay showed that L929 cells proliferated better on zein film than on glass on the third day after seeding and reached the peak one day earlier than on glass, although both assay methods proved that zein has a better biocompatibility. We noted that the background difference between glass and zein film was more highly significant in the MTT assay than in the CCK-8 assay, which means that the result of the CCK-8 assay was more credible.

To investigate the reason for the high background of the zein film in the MTT assay, we immersed glass slides and zein film slides either in PBS or in culture medium and performed the MTT assay. Table 4 shows the result. The background OD when immersed in culture medium was higher than that in PBS for both glass slides and zein film slides. Moreover, the background OD on the zein film slides that were immersed in either solution and incubated with MTT was much higher. For example, the background OD on the glass slides incubated with MTT was  $0.045 \pm 0.001$  in PBS and  $0.063 \pm 0.002$  in culture medium, while the background OD on zein film slides

incubated with MTT was  $0.142 \pm 0.006$  in PBS and  $0.246 \pm 0.014$  in culture medium. We speculate that some components may exist in both the culture medium and the zein film, which affect the reduction reaction from MTT to formazan. In addition, zein film can absorb a considerable amount of culture medium, which is in accord with the conclusion of our previous study: that the zein film has a good swelling property in solution [19]. One such component might be cysteine, because it exists in both zein and culture medium, and has a strong reducing ability among all kinds of amino acids. It has been reported that *N*-acetylcysteine has the ability to reduce the MTT tetrazolium ring [13]. At the same time, we found that there was no background interference on collagen, a typical protein that contains no cysteine, in the MTT assay [20,21]—a result that supports our speculation.

#### 4. Conclusions

We established an effective, biochemical method to evaluate the purity of zein from different sources, namely SDS-PAGE. We also investigated the influence of different sterilization methods on zein, and compared the MTT assay with the CCK-8 assay for the assessment of cell compatibility for this promising biomaterial. The four sources of zein that we used appeared to have no significant differences in amino acid and peptide chain composition. Neither dry-heat sterilization nor moist-heat sterilization procedures significantly affected the peptide chains of the zein.  $\gamma$ -ray sterilization at 25 kGy is a suitable dosage for the procedure of porous zein scaffold sterilization. When using an MTT assay, the background of zein itself affects the results of cell proliferation, while a CCK-8 assay is much more suitable to assess cell proliferation on zein films or scaffolds. From a CCK-8 assay, we obtained the conclusion that cell proliferation was better on zein film than on glass, as was previously established.

#### Acknowledgements


The authors are grateful to the financial support provided by the International S&T Cooperation Program of China (2014DFG02330 and 2015DFG32730). We also thank the Shanghai Municipal Science and Technology Commission (13JC1403400 and 15540723900) and the Medical Engineering Cooperation Program of Shanghai Jiao Tong University (YG2013MS77 and YG2014ZD03).

#### Compliance with ethics guidelines

Yue Zhang, Wei-Ying Li, Run Lan, and Jin-Ye Wang declare that they have no conflict of interest or financial conflicts to disclose.

#### References

- [1] Gianazza E, Viglienghi V, Righetti PG, Salamini F, Soave C. Amino acid composition of zein molecular components. *Phytochemistry* 1977;16(3):315–7.
- [2] Shukal R, Munir C. Zein: the industrial protein from corn. *Ind Crop Prod* 2001;13(3):171–92.
- [3] Dong J, Sun Q, Wang J. Basic study of corn protein, zein, as a biomaterial in tissue engineering, surface morphology and biocompatibility. *Biomaterials* 2004;25(19):4691–7.

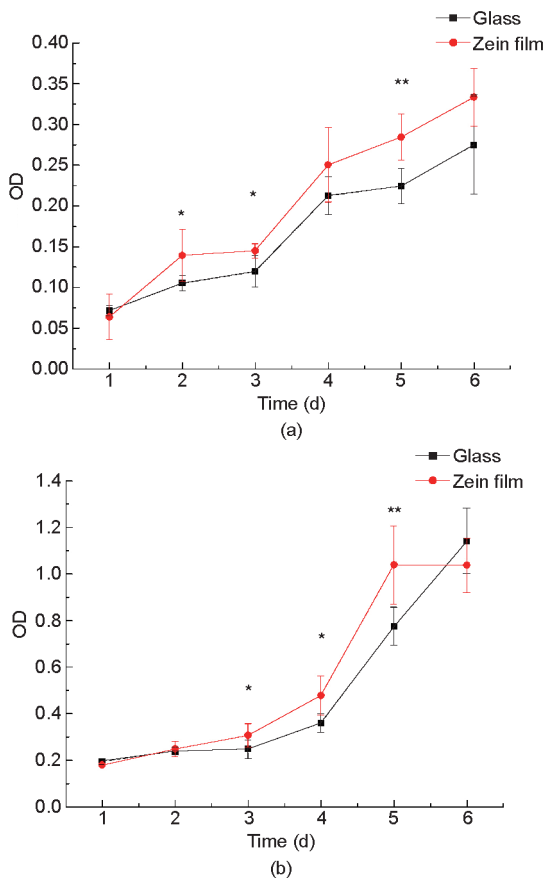

**Fig. 6.** Proliferation of L929 cells on glass and zein film. (a) The proliferation curve obtained from the MTT assay; (b) the proliferation curve obtained from the CCK-8 assay. \* indicates a significant difference (one-way ANOVA,  $P < 0.05$ ,  $n = 6$ ); \*\* indicates a highly significant difference (one-way ANOVA,  $P < 0.01$ ,  $n = 6$ ).

**Table 4**

OD of backgrounds on glass and zein film.

Surface	Glass slides				Zein film slides			
	PBS	Culture medium	PBS	Culture medium	PBS	Culture medium	PBS	Culture medium
MTT	–	+	–	+	–	+	–	+
OD (DMSO)	$0.044 \pm 0.003$	$0.045 \pm 0.001$	$0.050 \pm 0.001$	$0.063 \pm 0.002$	$0.045 \pm 0.001$	$0.142 \pm 0.006$	$0.054 \pm 0.001$	$0.246 \pm 0.014$

- [4] Gong S, Wang H, Sun Q, Xue S, Wang J. Mechanical properties and *in vitro* biocompatibility of porous zein scaffolds. *Biomaterials* 2006;27(20):3793–9.
- [5] Wang H, Gong S, Lin Z, Fu J, Xue S, Huang J, et al. *In vivo* biocompatibility and mechanical properties of porous zein scaffolds. *Biomaterials* 2007;28(27):3952–64.
- [6] Wang J, Wang H, Gong S. Preparation of zein scaffold for tissue engineering. In: Proceedings of the 8th World Biomaterials Congress; 2008 May 28–Jun 1; Amsterdam, the Netherlands. North Miami Beach: Curran Associates, Inc.; 2008. p. 4:1787.
- [7] Phillip E Jr, Murthy NS, Bolikal D, Narayanan P, Kohn J, Lavelle L, et al. Ethylene oxide's role as a reactive agent during sterilization: effects of polymer composition and device architecture. *J Biomed Mater Res-A* 2013;101(4):532–40.
- [8] Lee MH, Kim HL, Kim CH, Lee SH, Kim JK, Lee SJ, et al. Effects of low temperature hydrogen peroxide gas on sterilization and cytocompatibility of porous poly(*D,L*-lactic-co-glycolic acid) scaffolds. *Surf Coat Tech* 2008;202(22–23):5762–7.
- [9] Faraj KA, Brouwer KM, Geutjes PJ, Versteeg EM, Wismans RG, Deprest JA, et al. The effect of ethylene oxide sterilisation, beta irradiation and gamma irradiation on collagen fibril-based scaffolds. *Tissue Eng Regen Med* 2011;8(5):460–70.
- [10] Rnjak-Kovacina J, DesRochers TM, Burke KA, Kaplan DL. The effect of sterilization on silk fibroin biomaterial properties. *Macromol Biosci* 2015;15(6):861–74.
- [11] Zhang Z, Chen W. Plating densities, alpha-difluoromethylornithine effects and time dependence on the proliferation of IEC-6 cells. *China Med J* 2002;115(4):518–20.
- [12] Cetin Y, Bullerman LB. Evaluation of reduced toxicity of zearalenone by extrusion processing as measured by the MTT cell proliferation assay. *J Agr Food Chem* 2005;53(16):6558–63.
- [13] Bruggisser R, von Daeniken K, Jundt G, Schaffner W, Tullberg-Reinert H. Interference of plant extracts, phytoestrogens and antioxidants with the MTT tetrazolium assay. *Planta Med* 2002;68(5):445–8.
- [14] Fischer J, Prosenic MH, Wolff M, Hort N, Willumeit R, Feyerabend F. Interference of magnesium corrosion with tetrazolium-based cytotoxicity assays. *Acta Biomater* 2010;6(5):1813–23.
- [15] Tominaga H, Ishiyama M, Ohseto F, Sasamoto K, Hamamoto T, Suzuki K, et al. A water-soluble tetrazolium salt useful for colorimetric cell viability assay. *Anal Commun* 1999;36(2):47–50.
- [16] Jia J, Zhao X. GB/T 5009.124–2003 Determination of amino acids in foods. Beijing: Standards Press of China. 2003 Aug 11. Chinese.
- [17] Wang L, Huang Q, Wang J. Nanostructured polyaniline coating on ITO glass promotes the neurite outgrowth of PC 12 cells by electrical stimulation. *Langmuir* 2015;31(44):12315–22.
- [18] ISO 11137-1:2006 Sterilization of health care products—Radiation—Part 1: requirements for development, validation and routine control of a sterilization process for medical devices. Geneva: International Organization for Standardization; 2006 Apr 15.
- [19] Han Y, Xu Q, Lu Z, Wang J. Preparation of transparent zein films for cell culture applications. *Colloid Surface B* 2014;120(8):55–62.
- [20] Peng F, Wu H. 620 nm red light promotes cellular viability and mRNA expression of collagen type-I in bone mesenchymal stem cells of rat. In: SOPO 2010: Proceedings of the Symposium on Photonics and Optoelectronic; 2010 Jun 19–21; Chengdu, China. New Jersey: IEEE; 2010. p. 1–3.
- [21] Yan T, Sun R, Li C, Tan B, Mao X, Ao N. Immobilization of type-I collagen and basic fibroblast growth factor (bFGF) onto poly (HEMA-co-MMA) hydrogel surface and its cytotoxicity study. *J Mater Sci-Mater Med* 2010;21(8):2425–33.